

Unistat 912w

Unistat 912w controls the process temperature in a 30l DW reactor from AGI Glassplant

Requirement

This case study demonstrates the control capabilities over the process temperature when a Unistat 912w is connected with an AGI Glassplant 30l DW reactor.

Method

The Unistat 912w was connected to a 30l DW reactor from AGI Glassplant via 2 x 1,5m metal insulated tubes. The HTF used was Huber's M90.055/170.02 and the process mass simulated with 20l of Huber's DW-Therm.

Setup details


Temperature range:	-90°C...+250°C
Cooling power:	7.0 kW @ +20°C
	7.0 kW @ 0°C
	7.0 kW @ -20°C
Heating power:	6 kW
Hoses:	2 x 1,5m M30 metal Insulated
HTF:	M90.055/170.02
Reactor:	30l DW reactor AGI Glassplant
Reactor content:	20l DW-Therm
Stirrer speed:	150 rpm
Control:	process
Amb. temperature:	+23°C



Results

1. Lowest achievable temperature (Tmin):

The graphic below shows that the minimum achievable process temperature was -86.8°C with a corresponding jacket temperature of -88.6°C.

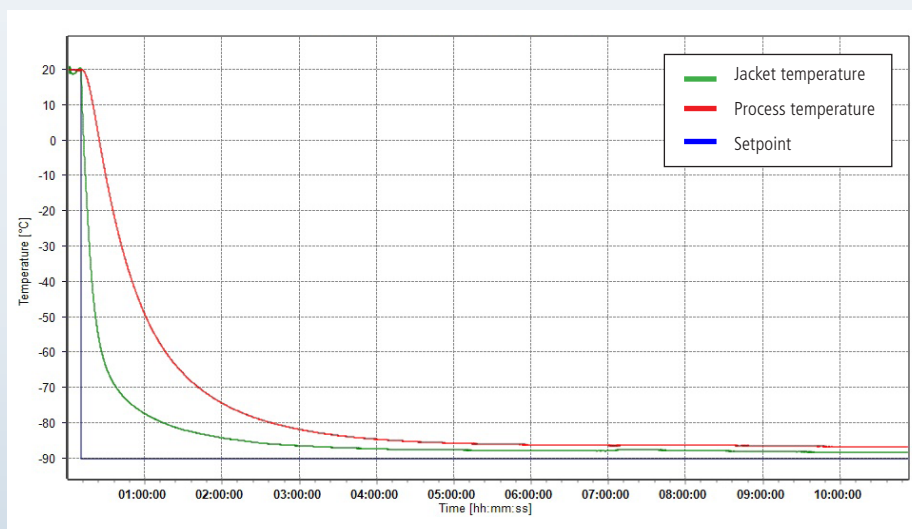

2. Performance: Temperature Control

The graphic below shows the speed, accuracy and stability as the Unistat 912w as it reaches and maintains each new set-point over a temperature range of -70°C to +100°C.

Start T	End T	Approximate time	Av. Ramp Rate
+20°C	-70°C	90 minutes	1.0 K/min
-70°C	+100°C	102 minutes	1.4 K/min
+100°C	+20°C	36 minutes	2.2 K/min

